


CLASSIC SERIES | Tuff™

BONE LEVEL IMPLANT



Bone Types	All bone types
PROSTHETICS PLATFORM	Internal hex
DESIGN FEATURES	<ul style="list-style-type: none"> • Moderate tapered body and tapered core • Double threads with a large step • Condensing variable threads design • Double flutes
CLINICAL BENEFITS	<ul style="list-style-type: none"> • Self tapping • High primary stability • Minimal drilling • Fast insertion – optimal for soft bone • Immediate loading - suitable for extraction sites

ORDERING INFORMATION

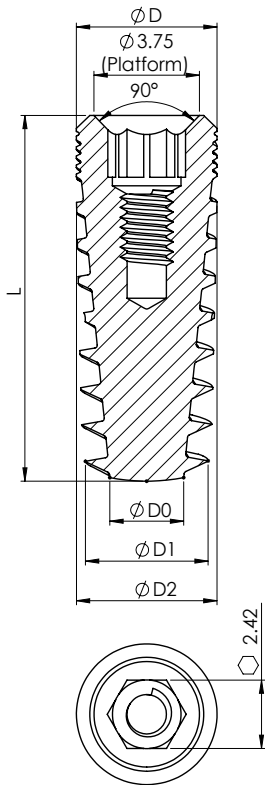


Ø D2 (mm)	Ø D0 (mm)	Ø D1 (mm)	Ø D (mm)	L (mm)	Ref. No
3.3	1.5	2.6	3.7	8	NM-F3308
				10	NM-F3310
				11.5	NM-F3311
				13	NM-F3313
				16	NM-F3316
3.75	1.8	3.1	3.8	6	NM-F3706
				8	NM-F3708
				10	NM-F3710
				11.5	NM-F3711
				13	NM-F3713
				16	NM-F3716
				18	NM-F3718
4.2	2.1	3.5	4.2	6	NM-F4206
				8	NM-F4208
				10	NM-F4210
				11.5	NM-F4211
				13	NM-F4213
				16	NM-F4216
				18	NM-F4218
				20	NM-F4220
				22	NM-F4222
				25	NM-F4225
5.0	2.7	4.5	5.0	6	NM-F5006
				8	NM-F5008
				10	NM-F5010
				11.5	NM-F5011
				13	NM-F5013
				16	NM-F5016
6.0	3.8	5.2	6.0	6	NM-F6006
				8	NM-F6008
				10	NM-F6010
				11.5	NM-F6011
				13	NM-F6013
				16	NM-F6016




CLASSIC SERIES | Tuff™

RECOMMENDED STRAIGHT DRILL PROTOCOL

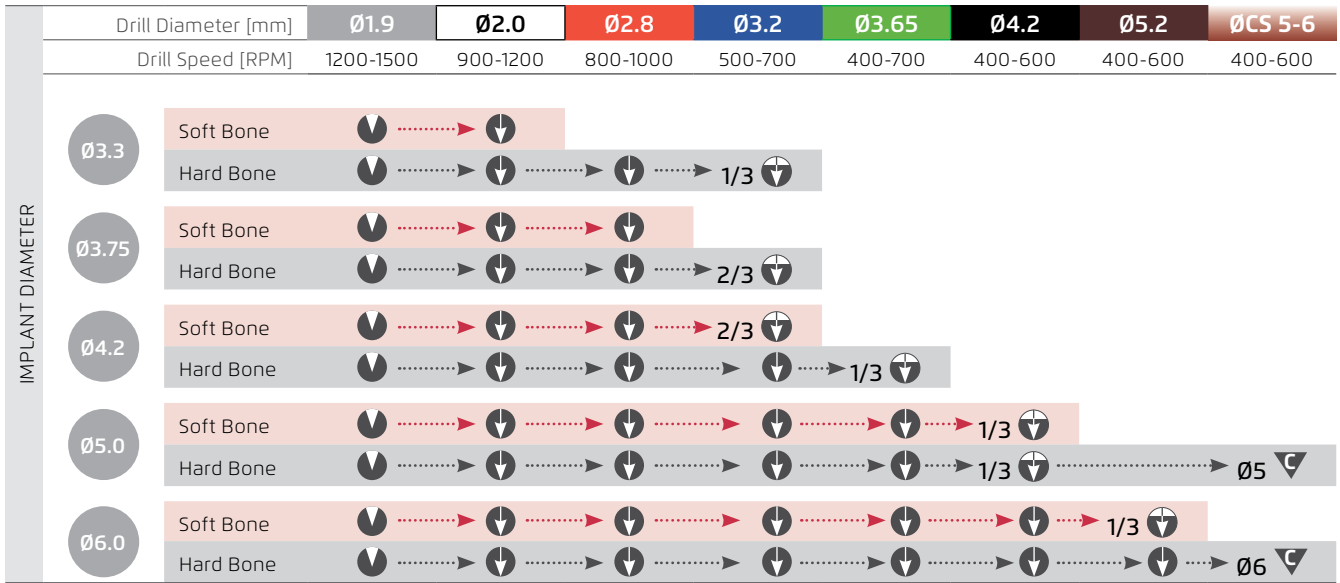


RECOMMENDED STEP DRILL PROTOCOL

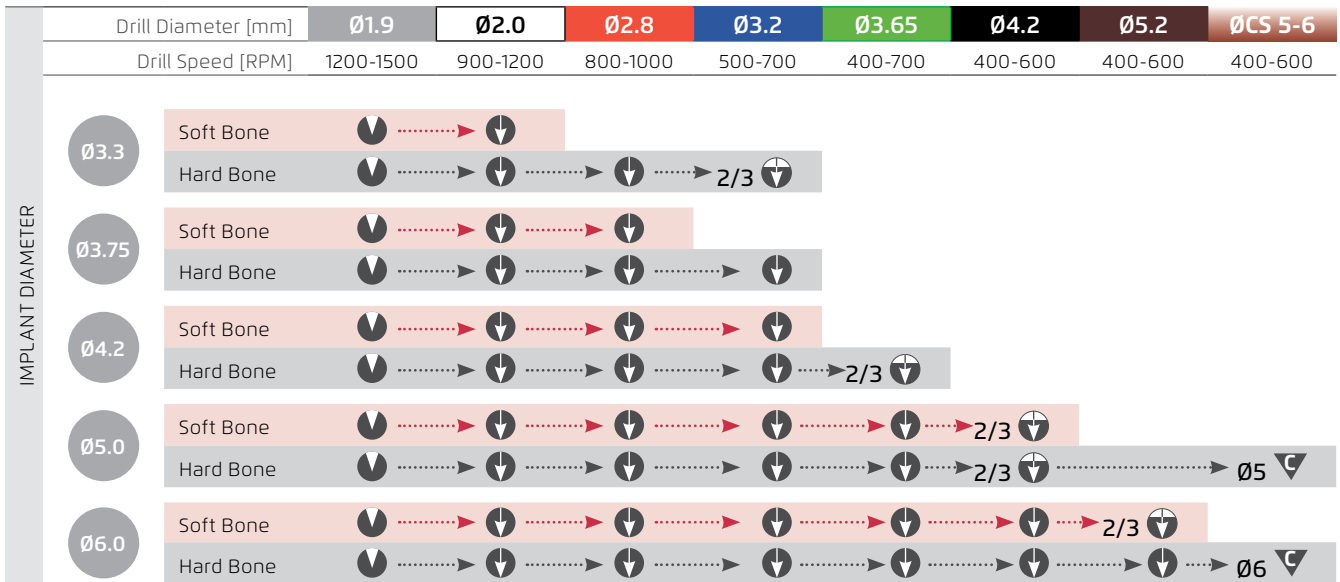

 Drill to mark osteotomy site	 Drill osteotomy to implant	 Drill osteotomy partially according to implant	 Drill with countersink to prepare the crest
--	--	--	---

The recommended drill protocol procedure should not replace the dentist's/surgeon's judgment. The implants may be loaded for immediate function when good primary stability (above 35 Ncm) has been achieved and with appropriate occlusal loading.

 For Implants longer than 16mm please refer to Long Drills page